



NMBAQC

NE Atlantic Marine Biological Analytical Quality Control Scheme

NMBAQC Scheme 2024/25

PS95 Report

Lydia McIntyre-Brown



Client: North East Atlantic Marine Biological Analytical Quality Control Scheme

Date of issue: 19/05/2025

Component Manager: Claire Mason (Cefas)

Project Manager: David Hall (Apem Ltd)

Component Administrator: Lydia McIntyre-Brown (Apem Ltd)

This report should be cited as:

McIntyre-Brown, L. & Hall, D., 2025. National Marine Biological Analytical Quality Control Scheme. Particle Size Results: PS95 Report to the NMBAQC Scheme participants. Apem Report NMBAQCps95, 18pp, May 2025.

Revision and Amendment Register

Version Number	Version Type	Date	Section(s)	Page(s)	Summary of Changes	Approved by
1.0	Interim	02/05/2025	All	All		LMB
1.1	Interim	12/05/2025	All	All	PSA_3115 results added	LMB
2.0	Final	09/05/2025	All	All		LMB

Contents

1.	BENCHMARK DATA.....	1
2.	PARTICIPANT DATA	9
3.	APPENDICES.....	17
	Appendix 1 – Participant Laser Replicate Graphs.....	17
	Appendix 2 – Gradistat output of size categories based on final merged data provided by each participant and the Benchmark Average for sediment distributed as PS95.	18
	Appendix 3 – Benchmark Lab and Participant Final Merged Data for sediment distributed as PS95.	18
	Appendix 4 – Individual comparison of participant and Benchmark sieve data for sediment distributed as PS95.	18

Figures

Figure 1 Particle size distribution curves resulting from sieve analysis of 5 replicate samples of sediment distributed as PS95 (Benchmark Data)	2
Figure 2 Particle size distribution curves resulting from final laser analysis of 5 replicate samples of sediment distributed as PS95 (Benchmark Data)	4
Figure 3 Particle size distribution curves resulting from laser analysis of five replicate samples of sediment distributed as PS95.	6
Figure 4 Particle size distribution curves resulting from analysis of 5 replicate samples of sediment distributed as PS95 (Benchmark Data).	8
Figure 5 Final sieve data (in percentages) provided by each participant for sediment distributed as PS95.....	12
Figure 6 Final laser data (in percentages) provided by each participant and the Benchmark average for sediment distributed as PS95.	14
Figure 7 Particle size distribution curves from all participating laboratories and the Benchmark average for sediment distributed as PS95.....	15
Figure 8 Bar charts showing the percentage gravel, sand, silt and clay recorded by each participating laboratory and the Benchmark average for PS95	16
Figure 9 Bar charts showing the percentage medium, fine and very fine gravel, sand, silt and clay recorded by each participating laboratory and the Benchmark average for PS95.	16

Tables

Table 1 Summary data for the Benchmark replicates distributed as PS95.	1
Table 2 Summary of the sieve data the Benchmark replicates distributed as PS95.	1
Table 3 Summary of the final laser data for the Benchmark replicates distributed as PS95.	3
Table 4 Summary of Coefficient of Variation for Benchmark laser replicates for PS95.	5
Table 5 Laser Metadata for the Benchmark replicates for PS95.	5
Table 6 Summary of equipment and methods used by participants and sample summary data provided by participants for sediment distributed as PS95.	9
Table 7 Summary of the sieve data provided by participants for sediment distributed as PS95.	10
Table 8 Summary of final laser data for the participants for sediment distributed as PS95 with Gradistat output.	13

Abbreviations

a/d – awaiting data – Deadline Extension Agreed

n/p – not participating at the current time.

n/r – no response from participant/ no data submitted.

“ – “ – no data submitted.

1. BENCHMARK DATA

Table 1 Summary data for the Benchmark replicates distributed as PS95.

Sample	Method	% Gravel	% Sand	% Mud	Sediment Description
PSA_3136 BM REP 1	NMBAQC	94.70	4.91	0.39	Gravel
PSA_3137 BM REP2	NMBAQC	94.68	4.99	0.33	Gravel
PSA_3138 BM REP 3	NMBAQC	94.74	4.96	0.30	Gravel
PSA_3139 BM REP 4	NMBAQC	94.66	4.98	0.36	Gravel
PSA_3140 BM REP 5	NMBAQC	94.50	5.17	0.33	Gravel
BM Rep Average	NMBAQC	94.66	5.00	0.34	Gravel

Table 2 Summary of the sieve data the Benchmark replicates distributed as PS95.

Phi Interval; microns	PSA_3036 BM REP 1	PSA_3037 BM REP2	PSA_3038 BM REP 3	PSA_3039 BM REP 4	PSA_3040 BM REP 5	BM Rep Average
Starting Weight >1mm	695.50	696.91	694.68	694.84	695.47	695.48
-6.50 to -6.00; 63 mm	0.00	0.00	0.00	0.00	0.00	0.00
-6.00 to -5.50; 45 mm	0.00	0.00	0.00	0.00	0.00	0.00
-5.50 to -5.00; 31.5 mm	0.00	0.00	0.00	0.00	0.00	0.00
-5.00 to -4.50; 22.4 mm	0.00	0.00	0.00	0.00	0.00	0.00
-4.50 to -4.00; 16 mm	0.00	0.00	0.00	0.00	0.00	0.00
-4.00 to -3.50; 11.2 mm	0.00	0.00	0.00	0.00	0.00	0.00
-3.50 to -3.00; 8 mm	0.00	0.00	0.00	0.00	0.00	0.00
-3.00 to -2.50; 5.6 mm	122.13	122.98	120.99	131.30	117.99	123.08
-2.50 to -2.00; 4 mm	471.33	468.59	464.02	453.92	461.01	463.77
-2.00 to -1.50; 2.8 mm	38.22	41.84	46.43	46.65	51.41	44.91
-1.50 to -1.00; 2 mm	31.71	31.13	31.16	31.65	32.54	31.64
-1.00 to -0.50; 1.4 mm	13.99	15.19	15.62	14.40	14.48	14.74
-0.50 to 0.00; 1.0 mm	16.42	15.87	15.22	16.32	17.16	16.20

Summary Data

>1.0mm	693.80	695.60	693.44	694.24	694.59	694.33
<1.0mm	Base Pan	1.83	1.39	1.26	0.96	1.29
	Oven dried	4.87	4.92	4.66	5.75	5.23
	Total	6.70	6.31	5.92	6.71	6.52
Total Weight	700.50	701.91	699.36	700.95	701.54	700.85
% increase/ decrease	0.02	0.01	0.00	0.05	0.02	0.02

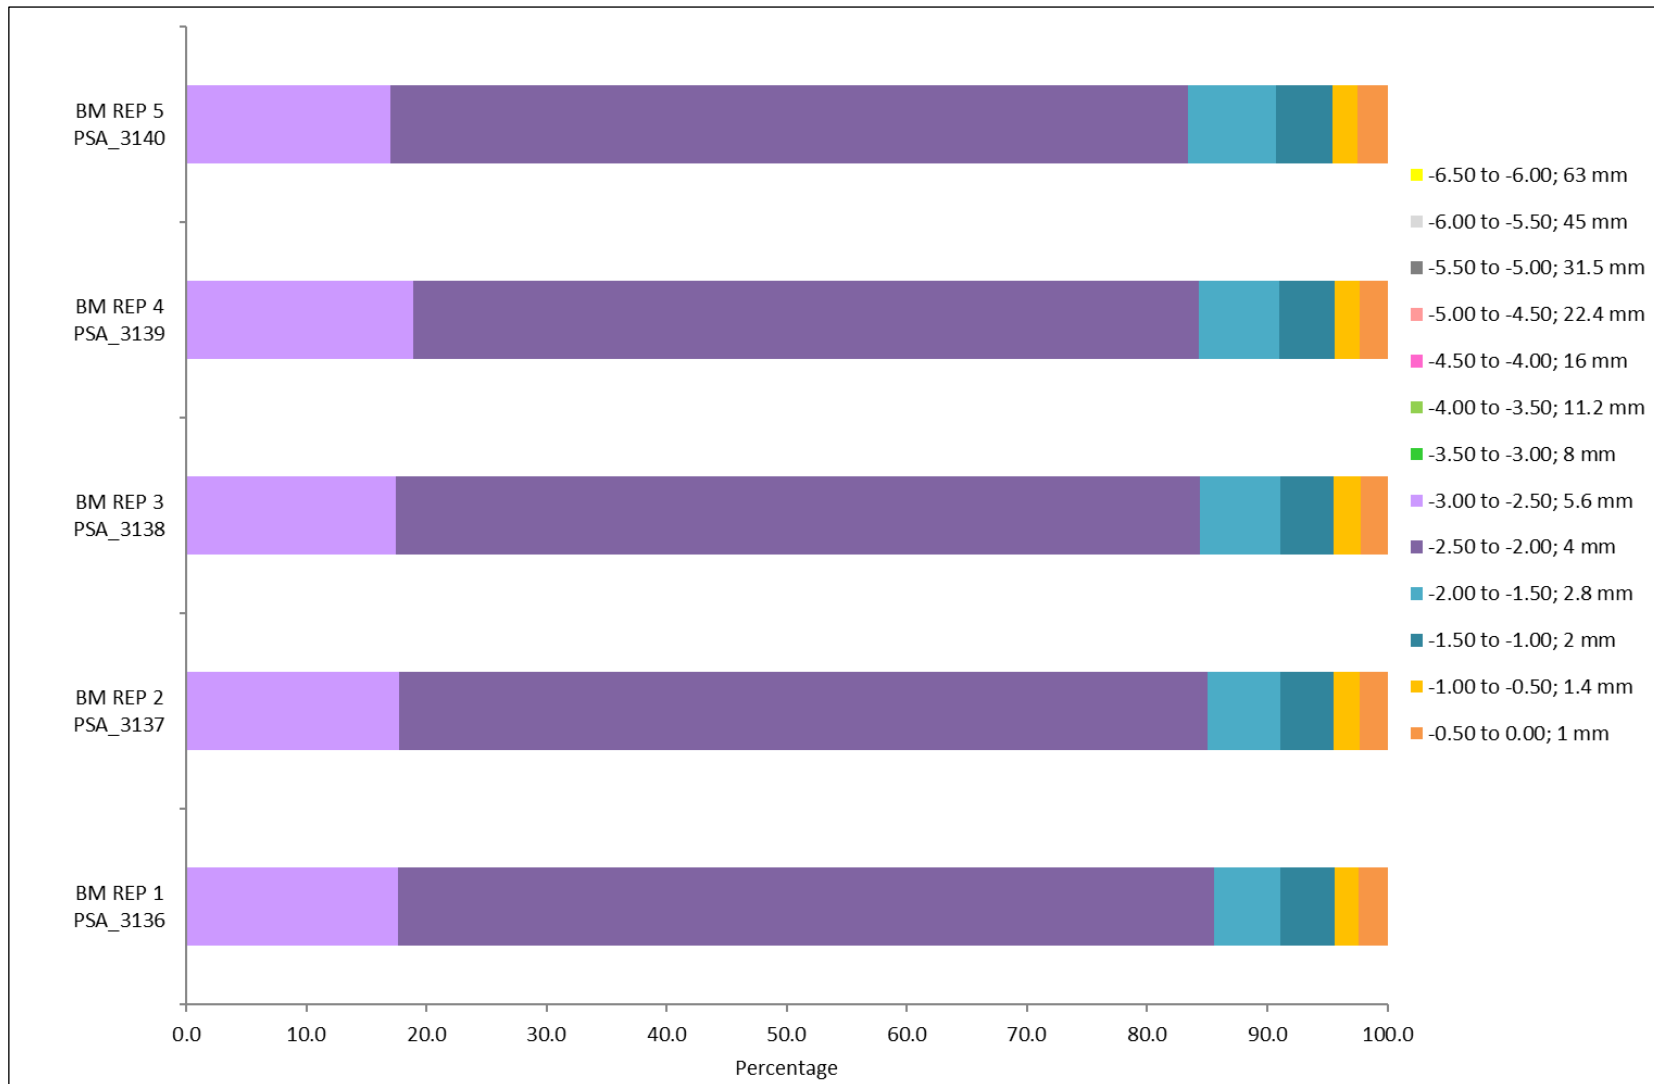


Figure 1 Particle size distribution curves resulting from sieve analysis of 5 replicate samples of sediment distributed as PS95 (Benchmark Data)

Table 3 Summary of the final laser data for the Benchmark replicates distributed as PS95.

Phi Interval; microns	PSA_3136 BM REP 1	PSA_3137 BM REP2	PSA_3138 BM REP 3	PSA_3139 BM REP 4	PSA_3140 BM REP 5	BM Rep Average
0.00 to 0.50; (707 μm)	28.09	26.87	30.41	27.88	30.88	28.83
0.50 to 1.00; (500 μm)	8.66	11.42	10.85	10.35	12.39	10.74
1.00 to 1.50; (353.6 μm)	7.18	8.37	7.66	7.16	7.77	7.63
1.50 to 2.00; (250 μm)	5.04	6.38	6.09	6.07	5.78	5.87
2.00 to 2.50; (176.8 μm)	3.46	3.76	3.15	3.41	3.45	3.45
2.50 to 3.00; (125 μm)	2.29	2.30	2.32	2.76	2.49	2.43
3.00 to 3.50; (88.39 μm)	2.35	2.24	2.30	2.64	2.43	2.39
3.50 to 4.00; (62.5 μm)	2.07	1.74	1.66	1.78	1.60	1.77
4.00 to 4.50; (44.19 μm)	2.36	2.13	1.86	2.09	2.07	2.10
4.50 to 5.00; (31.25 μm)	3.81	3.15	3.03	3.12	2.91	3.20
5.00 to 5.50; (22.097 μm)	4.18	3.64	3.51	3.60	3.33	3.65
5.50 to 6.00; (15.625 μm)	4.21	3.85	3.61	3.80	3.52	3.80
6.00 to 6.50; (11.049 μm)	4.47	4.06	3.94	4.06	3.67	4.04
6.50 to 7.00; (7.813 μm)	3.92	3.61	3.48	3.68	3.19	3.58
7.00 to 7.50; (5.524 μm)	3.60	3.26	3.19	3.38	2.91	3.27
7.50 to 8.00; (3.906 μm)	3.24	2.89	2.87	3.04	2.59	2.93
8.00 to 8.50; (2.762 μm)	2.59	2.32	2.30	2.47	2.06	2.35
8.50 to 9.00; (1.953 μm)	2.04	1.85	1.85	1.99	1.64	1.87
9.00 to 9.50; (1.381 μm)	1.73	1.59	1.61	1.71	1.43	1.61
9.50 to 10.00; (0.977 μm)	1.44	1.33	1.36	1.44	1.21	1.36
10.00 to 10.50; (0.691 μm)	1.10	1.04	1.03	1.13	0.92	1.04
10.50 to 11.00; (0.488 μm)	0.78	0.76	0.72	0.83	0.65	0.75
11.00 to 11.50; (0.345 μm)	0.54	0.54	0.49	0.59	0.44	0.52
11.50 to 12.00; (0.244 μm)	0.36	0.37	0.32	0.41	0.29	0.35
12.00 to 12.50; (0.173 μm)	0.22	0.24	0.19	0.27	0.18	0.22
12.50 to 13.00; (0.122 μm)	0.14	0.16	0.12	0.18	0.11	0.14
13.00 to 13.50; (0.086 μm)	0.08	0.09	0.07	0.11	0.06	0.08
13.50 to 14.00; (0.061 μm)	0.03	0.04	0.02	0.04	0.02	0.03
14.00 to 14.50; (0.043 μm)	0.00	0.00	0.00	0.01	0.00	0.00
>14.50; (0.01 μm)	0.00	0.00	0.00	0.00	0.00	0.00
Total	100.00	100.00	100.00	100.00	100.00	100.00

Summary Data

Mean	106.41	121.16	128.76	113.92	141.72	122.24
Sorting	8.92	8.57	8.48	8.96	7.97	8.59
Skewness	-0.51	-0.60	-0.64	-0.58	-0.67	-0.61
Kurtosis	0.67	0.70	0.70	0.69	0.73	0.70
Mode	Bimodal	Bimodal	Unimodal	Unimodal	Unimodal	Unimodal
MODE 1 (μm)	853.5	853.5	853.5	853.5	853.5	853.5
MODE 2 (μm)	13.3	13.3	-	-	-	-

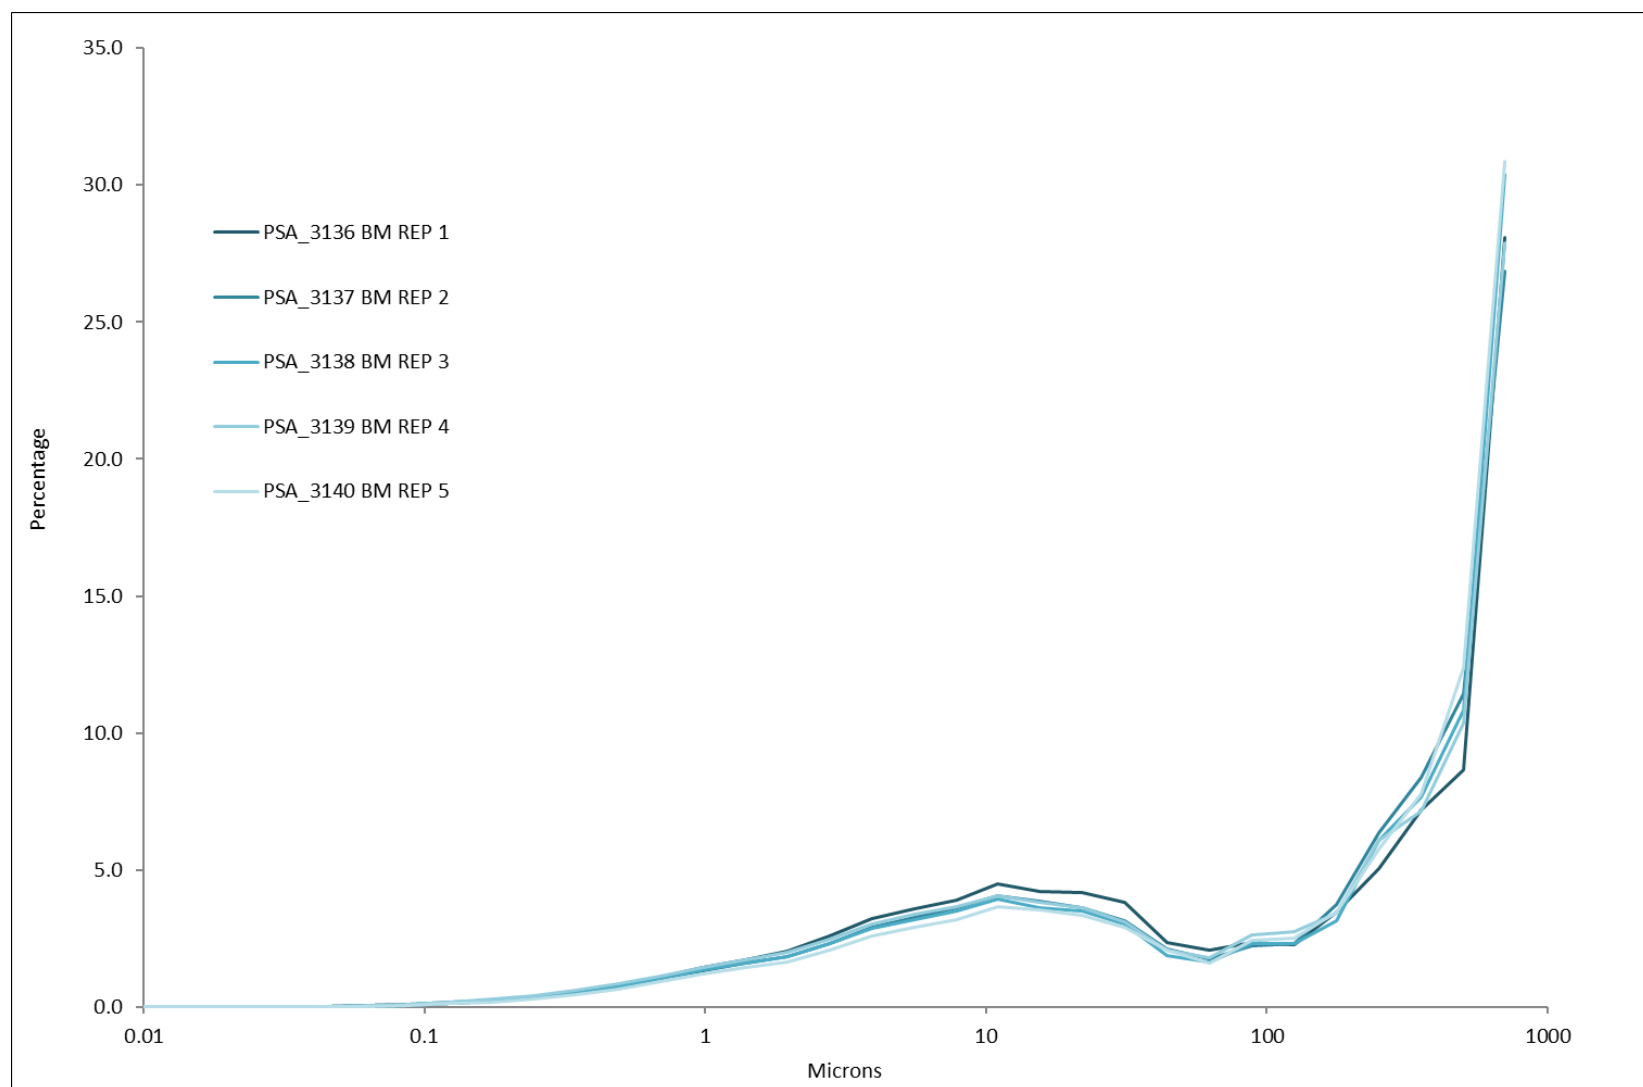


Figure 2 Particle size distribution curves resulting from final laser analysis of 5 replicate samples of sediment distributed as PS95 (Benchmark Data)

Table 4 Summary of Coefficient of Variation for Benchmark laser replicates for PS95.

		PSA_3136 BM REP 1	PSA_3137 BM REP2	PSA_3138 BM REP 3	PSA_3139 BM REP 4	PSA_3140 BM REP 5
D ₁₀	Sub-sample 1	1.86	1.34	1.45	2.71	3.44
	Sub-sample 2	2.41	4.47	4.64	3.94	1.78
	Sub-sample 3	5.03	0.46	2.55	2.79	2.55
D ₅₀	Sub-sample 1	7.87	4.16	2.69	5.29	4.78
	Sub-sample 2	2.67	3.67	3.68	5.71	4.20
	Sub-sample 3	7.04	1.84	4.38	1.64	1.02
D ₉₀	Sub-sample 1	0.36	0.55	0.11	0.18	0.22
	Sub-sample 2	0.23	0.49	0.17	0.26	0.56
	Sub-sample 3	0.06	0.25	0.37	0.24	0.29

$$COV = \left(\frac{StDev}{Mean} \right) * 100$$

ISO 133020 defines good reproducibility when: COV is <3% for D50

COV is <5% for D10 and D90

All limits double when the D50 is <10microns.

In reality 3% and 5% are low and greater variability is expected for natural sediment samples therefore a maximum of 20% (based on three replicates being measured) will be used as a guide.

The Benchmark replicates show good reproducibility.

Table 5 Laser Metadata for the Benchmark replicates for PS95.

	Benchmark Lab
Laser used:	Beckman Coulter LS 13320
Dispersion Unit:	Universal Liquid Module
Analysis model:	Mie
Dispersion Used	Water (RI – 1.33)
Particle Refractive Index	1.55
Particle Absorption Index:	0.1
Fines extension	PIDS system
Obscuration	10%
Pump Speed (% or rpm)	80%
Stirrer speed (% or rpm)	n/a
Ultrasonic duration	20
Ultrasonic level	2

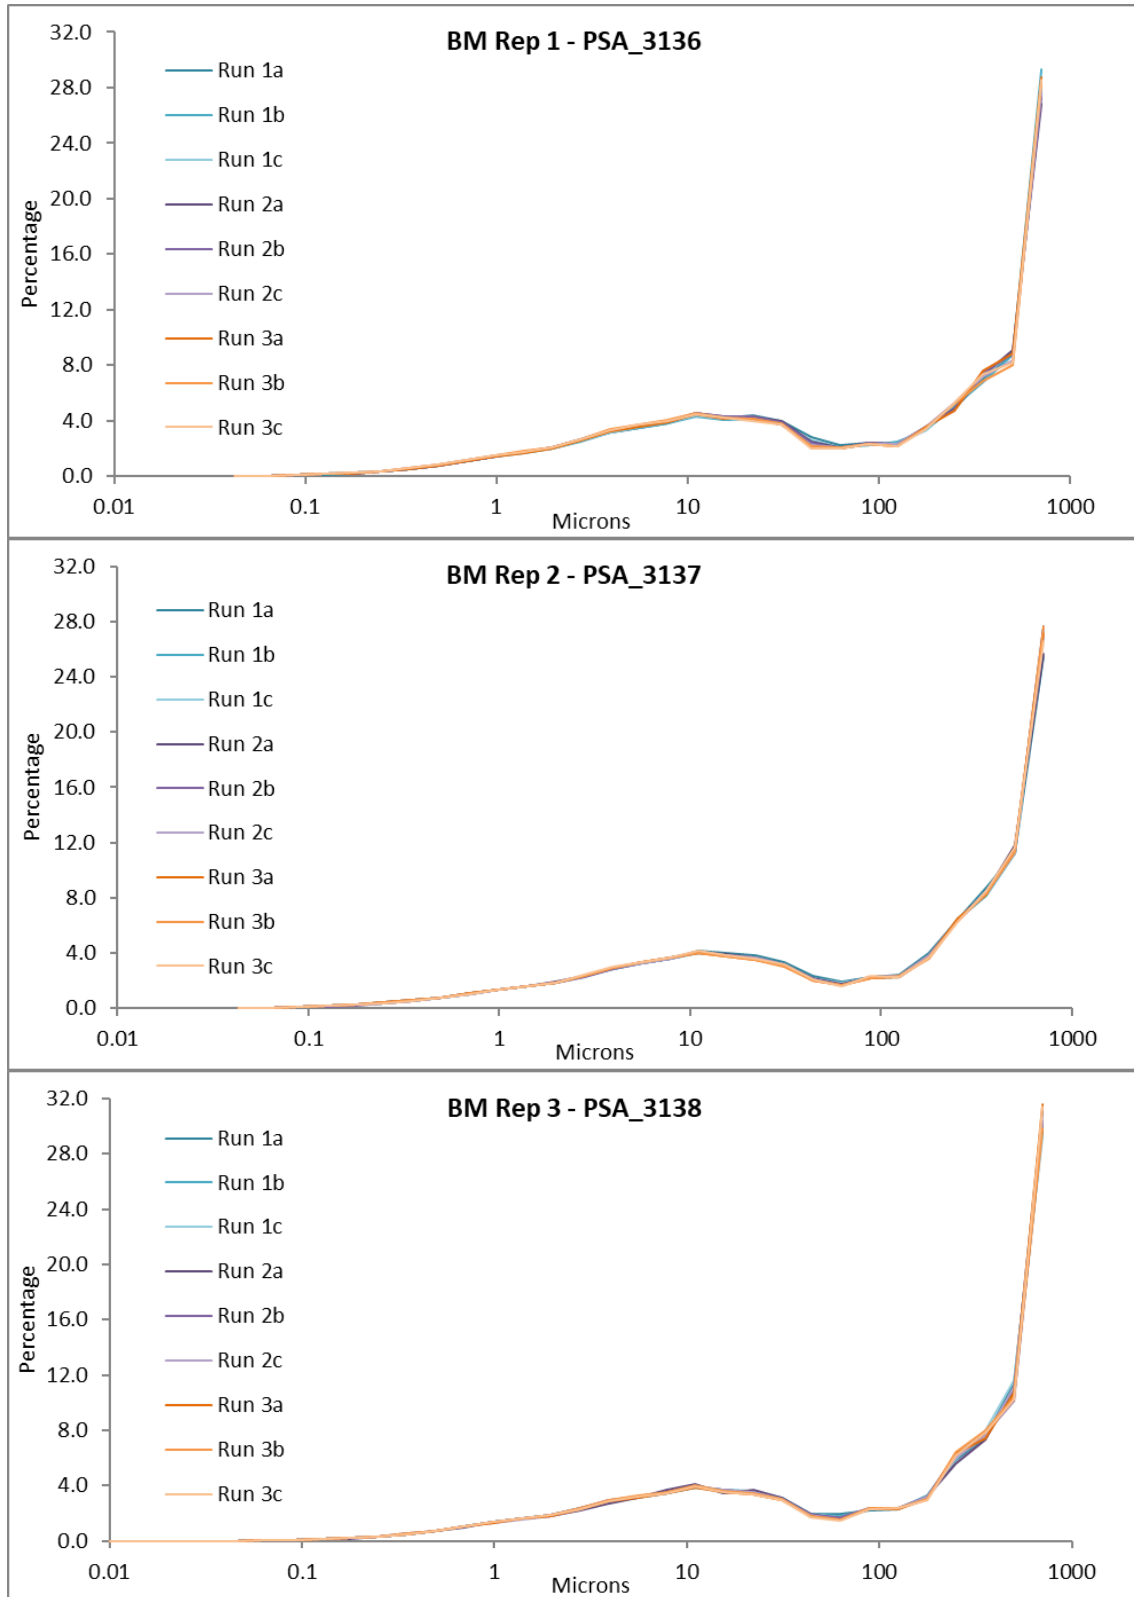


Figure 3 Particle size distribution curves resulting from laser analysis of five replicate samples of sediment distributed as PS95.

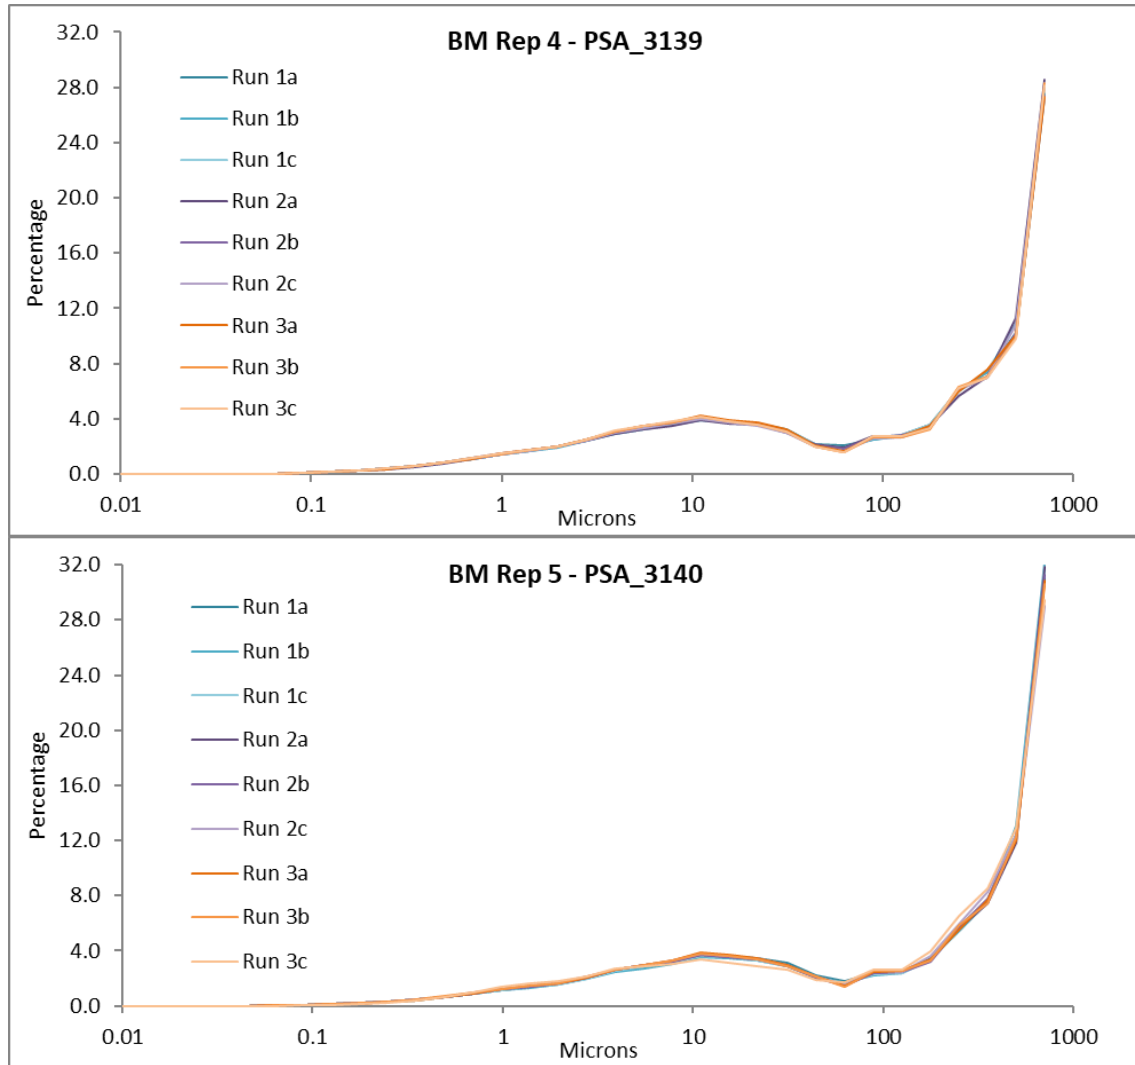


Figure 3 Particle size distribution curves resulting from laser analysis of five replicate samples of sediment distributed as PS95.

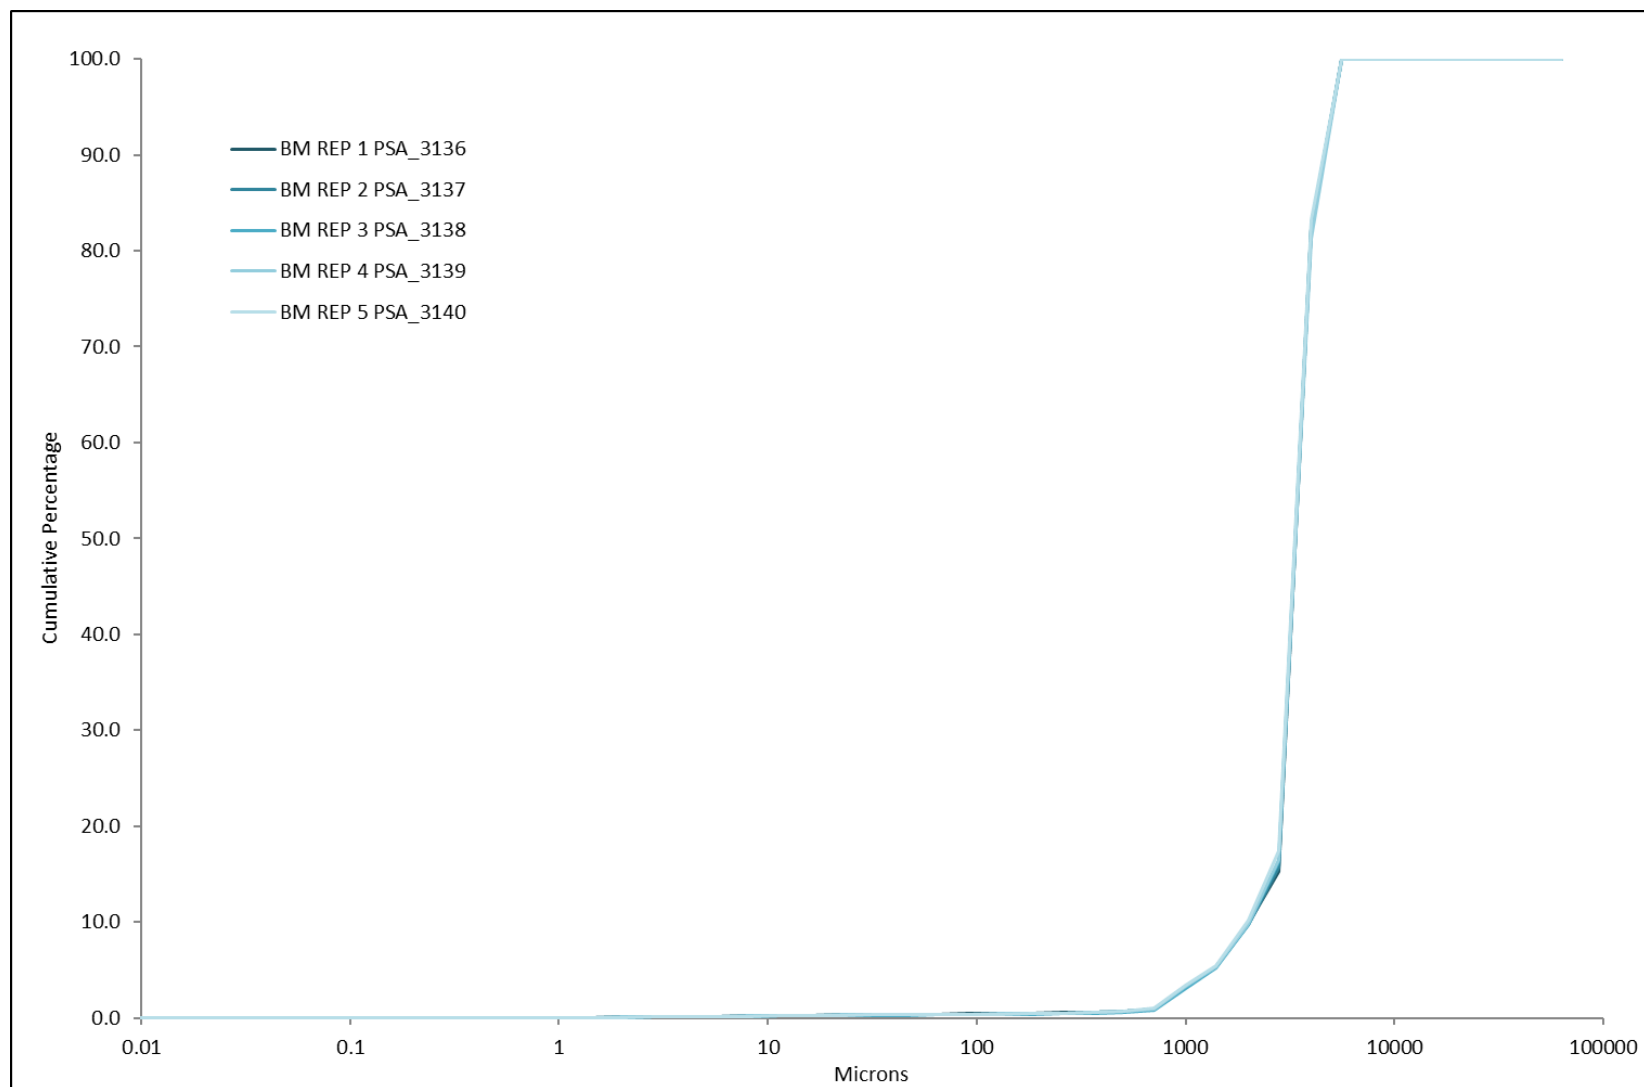


Figure 4 Particle size distribution curves resulting from analysis of 5 replicate samples of sediment distributed as PS95 (Benchmark Data).

2. PARTICIPANT DATA

Table 6 Summary of equipment and methods used by participants and sample summary data provided by participants for sediment distributed as PS95.

Lab	Equipment Used		Method Used	Chemical Dispersant	Peroxide pre-treatment	Summary Data			Sediment Description	
	Sieves	Laser				% Gravel	% Sand	% Mud	(post analysis)	Gradistat Textural Group
BM Average	Yes	Yes	NMBAQC	No	No	94.66	5.00	0.34	Gravel	Gravel
PSA_3101	Yes	No	NMBAQC	No	No	94.83	5.17	0.00	Gravel	Gravel
PSA_3102	Yes	No	NMBAQC	No	No	95.60	4.40	0.00	Gravel	Gravel
PSA_3103	Yes	Yes	NMBAQC	No	No	94.95	4.96	0.08	Gravel	Gravel
PSA_3104	Yes	No	NMBAQC	No	No	94.84	5.16	0.00	Coarse sediment	Gravel
PSA_3105	Yes	No	NMBAQC	No	No	95.20	4.80	0.00	Gravel	Gravel
PSA_3106	Yes	No	NMBAQC	No	No	94.31	5.67	0.02	Gravel	Gravel
PSA_3107	Yes	Yes	NMBAQC	No	No	94.81	4.92	0.27	Gravel	Gravel
PSA_3108_a	Yes	Yes	NMBAQC	No	No	94.66	4.94	0.40	Gravel	Gravel
PSA_3108_b	Yes	Yes	NMBAQC	No	No	94.64	5.02	0.34	Gravel	Gravel
PSA_3109	Yes	Yes	OTHER	No	No	95.96	3.70	0.34	Gravel	Gravel
PSA_3110	Yes	No	NMBAQC	No	No	95.02	4.98	0.00	Gravel	Gravel
PSA_3111	Yes	No	OTHER	No	No	94.74	5.26	0.00	Gravel	Gravel
PSA_3112	n/p	n/p	n/p	n/p	n/p	n/p	n/p	n/p	n/p	Gravel
PSA_3113	Yes	No	NMBAQC	No	No	97.02	2.99	0.00	Gravel	Gravel
PSA_3114	Yes	No	NMBAQC	No	No	95.60	4.40	0.00	Gravel	Gravel
PSA_3115	Yes	No	NMBAQC	No	No	94.79	5.21	0.00	Gravel	Gravel
PSA_3116	n/r	n/r	n/r	n/r	n/r	n/r	n/r	n/r	n/r	n/r
PSA_3117	n/r	n/r	n/r	n/r	n/r	n/r	n/r	n/r	n/r	n/r

Table 7 Summary of the sieve data provided by participants for sediment distributed as PS95.

Phi interval (explicit); Sieve mesh (mm)	BM Average	PSA_3101	PSA_3102	PSA_3103	PSA_3104	PSA_3105	PSA_3106	PSA_3107	PSA_3108_a	PSA_3108_b
Starting weight (>1.0mm)	695.48	696.36	693.85	696.42	692.65	696.39	705.25	692.39	694.42	694.84
-6.50 to -6.00; 63 mm	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.000	0.00
-6.00 to -5.50; 45 mm	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.000	0.00
-5.50 to -5.00; 31.5 mm	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.000	0.00
-5.00 to -4.50; 22.4 mm	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.000	0.00
-4.50 to -4.00; 16 mm	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.000	0.00
-4.00 to -3.50; 11.2 mm	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.000	0.00
-3.50 to -3.00; 8 mm	0.00	0.00	0.00	0.00	0.00	9.27	0.00	0.00	0.000	0.00
-3.00 to -2.50; 5.6 mm	123.08	187.13	135.21	121.41	133.93	237.31	149.50	136.77	146.659	123.08
-2.50 to -2.00; 4 mm	463.77	412.15	462.80	485.05	443.55	367.76	457.44	471.18	455.045	463.77
-2.00 to -1.50; 2.8 mm	44.91	33.58	30.83	25.40	48.06	22.59	24.70	23.44	25.701	44.91
-1.50 to -1.00; 2 mm	31.64	30.38	32.99	33.82	35.93	28.06	33.54	31.36	34.175	31.64
-1.00 to -0.50; 1.4 mm	14.74	15.52	14.37	13.71	13.09	18.66	13.79	13.21	12.653	14.74
-0.50 to 0.00; 1 mm	16.20	16.16	15.87	17.02	15.22	10.39	19.97	15.46	18.146	16.20
Total	694.33	694.92	692.07	696.42	689.78	694.04	698.93	691.42	692.38	694.33
Summary Data										
>1 mm	694.33	694.92	692.07	696.42	689.78	694.04	698.93	691.42	692.379	694.33
<1 mm	Base pan	1.29	1.66	1.86	4.66	3.07	2.22	6.35	1.23	1.29
	Oven dried	5.23	2.84	4.39	0.00	4.59	2.26	0.00	6.40	5.23
	Total	6.52	4.50	6.25	4.66	7.66	4.48	6.35	7.63	6.52
Total Sample Weight	700.85	699.42	698.32	701.07	697.44	696.30	705.28	699.05	698.921	699.018
% increase/ decrease	0.02	0.03	0.01	0.67	0.03	-0.01	0.89	0.04	0.01	-0.03

Table 7 Summary of the sieve data provided by participants for sediment distributed as PS95.

Phi interval (explicit); Sieve mesh (mm)	BM Average	PSA_3109	PSA_3110	PSA_3111	PSA_312	PSA_3113	PSA_3114	PSA_3115	PSA_3116	PSA_317
Starting weight (>1.0mm)	695.48	-	699.66	688.67	n/p	702.19	696.20	701.69	n/r	n/r
-6.50 to -6.00; 63 mm	0.00		0.00	0.00	n/p	0.00	0.00	0.00	n/r	n/r
-6.00 to -5.50; 45 mm	0.00		0.00	0.00	n/p	0.00	0.00	0.00	n/r	n/r
-5.50 to -5.00; 31.5 mm	0.00		0.00	0.00	n/p	0.00	0.00	0.00	n/r	n/r
-5.00 to -4.50; 22.4 mm	0.00		0.00	0.00	n/p	0.00	0.00	0.00	n/r	n/r
-4.50 to -4.00; 16 mm	0.00		0.00	0.00	n/p	0.00	0.00	0.00	n/r	n/r
-4.00 to -3.50; 11.2 mm	0.00		0.00	0.00	n/p	0.00	0.00	0.00	n/r	n/r
-3.50 to -3.00; 8 mm	0.00		0.00	0.00	n/p	0.00	1.22	0.00	n/r	n/r
-3.00 to -2.50; 5.6 mm	123.08		167.45	128.57	n/p	168.58	146.08	192.41	n/r	n/r
-2.50 to -2.00; 4 mm	463.77		440.60	386.80	n/p	442.65	456.90	420.05	n/r	n/r
-2.00 to -1.50; 2.8 mm	44.91	671.59	21.06	109.93	n/p	23.12	28.20	21.00	n/r	n/r
-1.50 to -1.00; 2 mm	31.64		35.70	34.50	n/p	33.06	30.90	31.70	n/r	n/r
-1.00 to -0.50; 1.4 mm	14.74	24.58	11.94	10.57	n/p	13.83	14.50	16.19	n/r	n/r
-0.50 to 0.00; 1 mm	16.20		17.40	18.30	n/p	16.41	16.00	16.47	n/r	n/r
Total	694.33	696.17	694.15	688.67	n/p	697.65	693.80	697.82	n/r	n/r
Summary Data										
>1 mm	694.33	696.17	694.15	688.67	n/p	697.65	693.80	697.82	n/r	n/r
<1 mm	Base pan	1.29	-	5.51	-	n/p	4.54	2.40	3.59	n/r
	Oven dried	5.23	-	-	7.77	n/p	0.00	2.96	-	n/r
	Total	6.52	-	5.51	7.77	n/p	4.54	5.36	3.59	n/r
Total Sample Weight	700.85	696.17	699.66	696.43	n/p	702.19	699.16	701.41	n/r	n/r
% increase/ decrease	0.02	-	0.00	-	n/p	0.00	0.00	-0.04	n/r	n/r

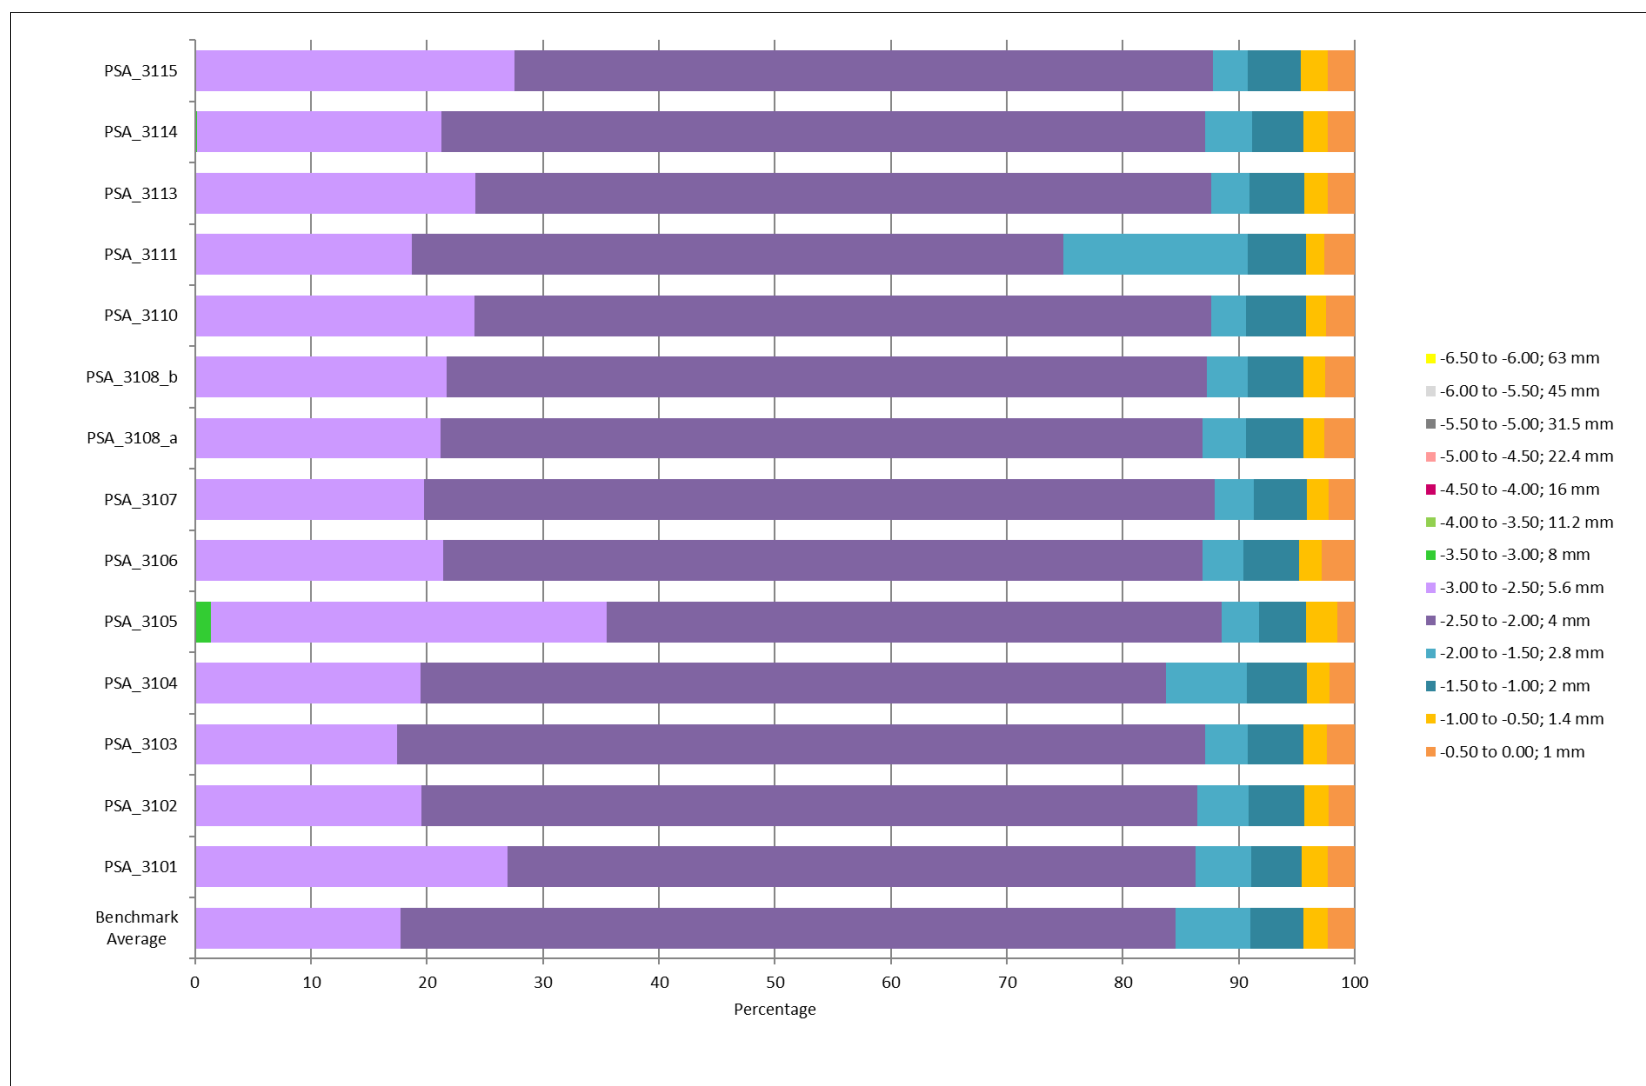


Figure 5 Final sieve data (in percentages) provided by each participant for sediment distributed as PS95.

Table 8 Summary of final laser data for the participants for sediment distributed as PS95 with Gradistat output.

Microns	BM Average	PSA_3103	PSA_3107	PSA_3108_a	PSA_3108_b	PSA_3109
1400	-	-	-	-	-	11.40
1000	-	-	-	-	-	10.89
707	28.83	40.16	45.90	24.28	23.85	3.45
500	10.74	24.61	16.06	16.79	17.99	0.10
353.6	7.63	9.20	5.89	6.41	9.12	0.00
250	5.87	3.08	4.64	1.33	3.95	0.31
176.8	3.45	2.94	1.36	0.92	2.69	3.85
125	2.43	3.27	0.40	1.82	2.72	4.95
88.39	2.39	2.58	0.01	2.58	2.73	0.67
62.5	1.77	1.79	1.00	3.09	2.76	0.00
44.19	2.10	1.52	1.56	3.63	2.99	3.43
31.25	3.20	1.54	1.40	4.10	3.26	7.72
22.097	3.65	1.51	2.67	4.28	3.31	9.06
15.625	3.80	1.35	2.15	4.20	3.15	8.29
11.049	4.04	1.17	3.04	4.04	2.97	6.91
7.813	3.58	1.04	2.12	3.94	2.90	5.71
5.524	3.27	0.95	2.22	3.88	2.96	4.91
3.906	2.93	0.86	2.50	3.75	3.01	4.38
2.762	2.35	0.75	1.42	3.36	2.84	3.88
1.953	1.87	0.61	1.19	2.69	2.39	3.23
1.381	1.61	0.46	1.41	1.93	1.77	2.47
0.977	1.36	0.34	1.07	1.33	1.23	1.85
0.691	1.04	0.24	0.61	0.97	0.86	1.44
0.488	0.75	0.02	0.38	0.60	0.51	0.93
0.345	0.52	0.00	0.29	0.10	0.05	0.19
0.244	0.35	0.00	0.24	0.00	0.00	0.00
0.173	0.22	0.00	0.19	0.00	0.00	0.00
0.122	0.14	0.00	0.14	0.00	0.00	0.00
0.086	0.08	0.00	0.09	0.00	0.00	0.00
0.061	0.03	0.00	0.04	0.00	0.00	0.00
0.043	0.00	0.00	0.01	0.00	0.00	0.00
0.01	0.00	0.00	0.00	0.00	0.00	0.00
Total	100.00	100.00	100.00	100.00	100.00	100.00
MEAN:	122.24	392.94	200.20	93.94	133.41	53.57
SORTING:	8.59	3.32	7.05	8.56	7.89	11.72
SKEWNESS:	-0.61	-0.73	-0.86	-0.40	-0.68	0.26
KURTOSIS:	0.70	1.99	0.99	0.64	0.73	0.64
MODE:	Unimodal	Unimodal	Unimodal	Bimodal	Unimodal	Trimodal
MODE 1 (µm):	853.50	853.5	853.5	853.5	853.5	1200.0
MODE 2 (µm):	-	-	-	26.7	-	26.7
MODE 3 (µm):	-	-	-	-	-	2.75

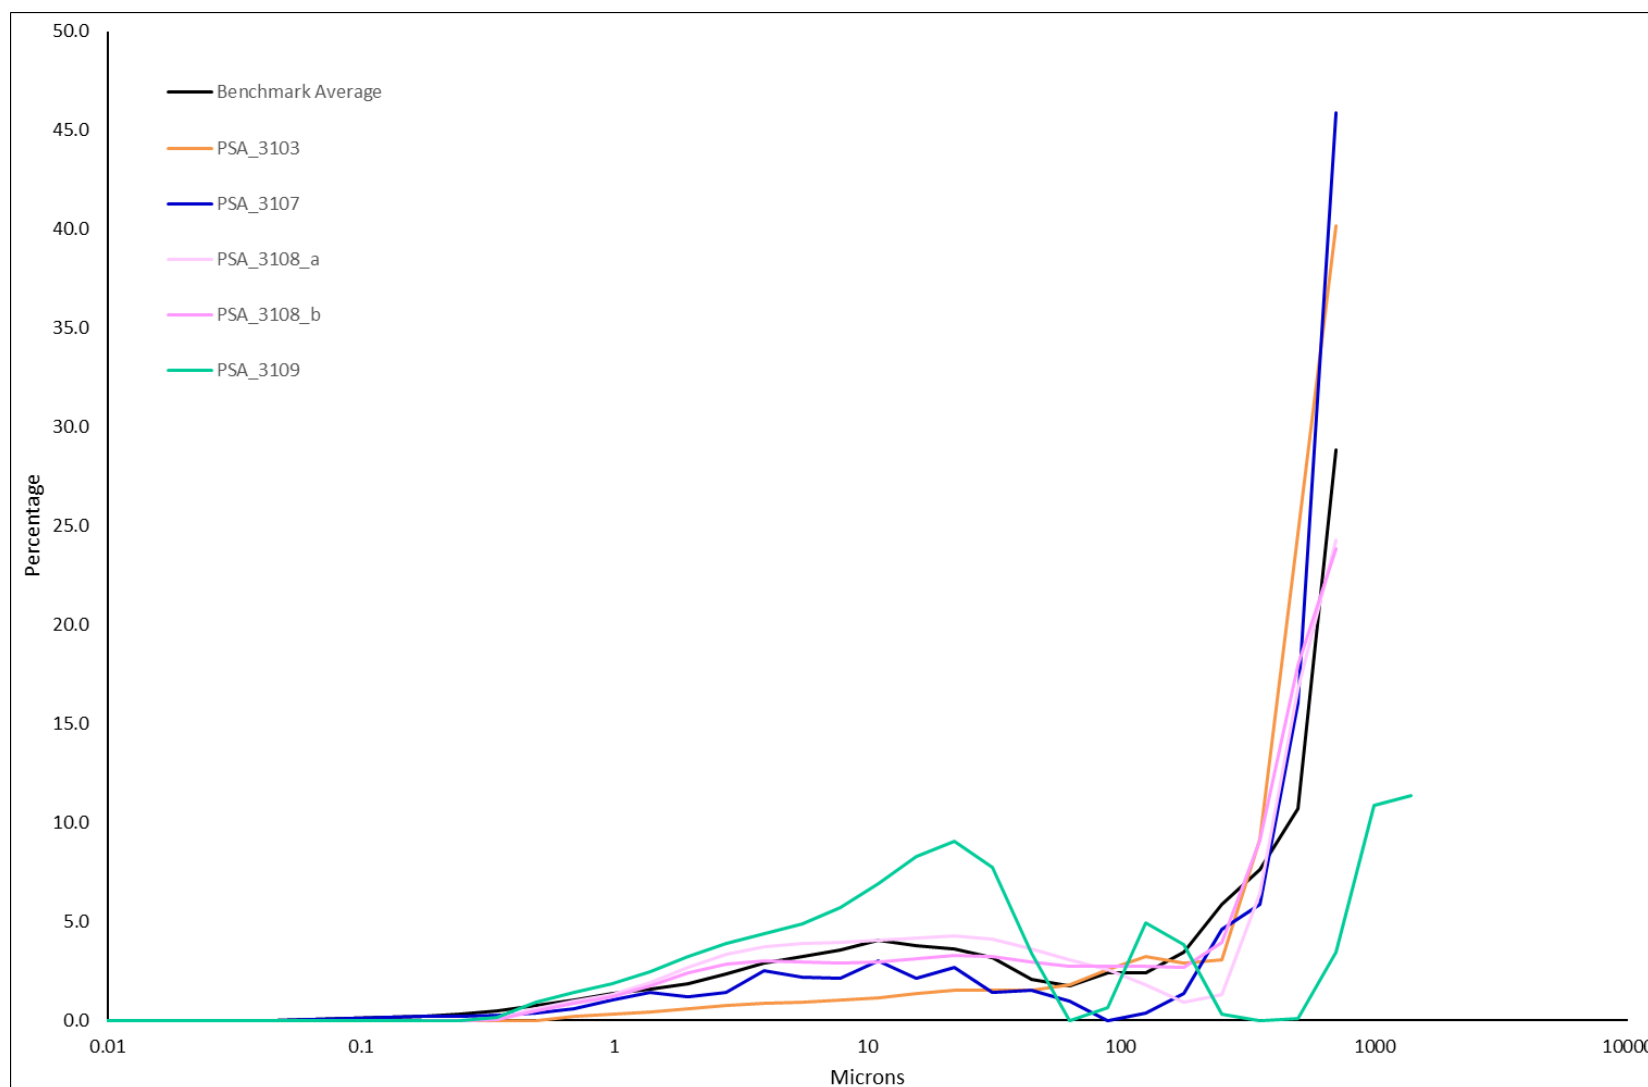


Figure 6 Final laser data (in percentages) provided by each participant and the Benchmark average for sediment distributed as PS95.

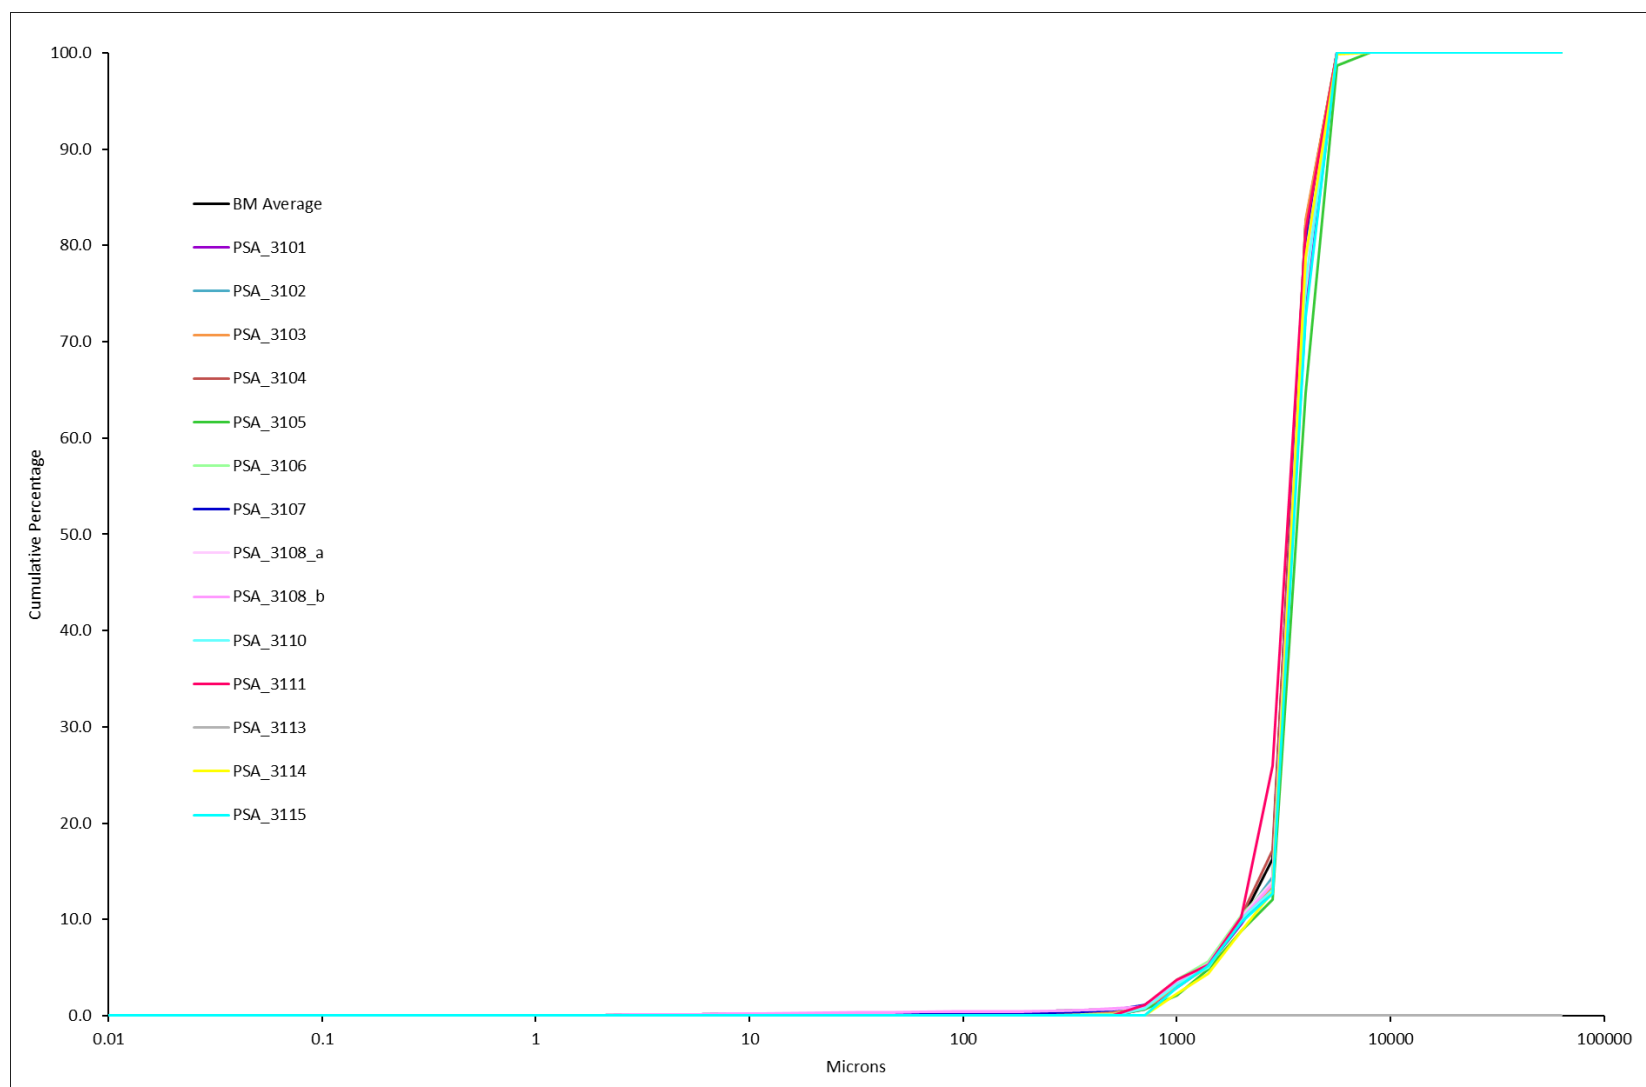


Figure 7 Particle size distribution curves from all participating laboratories and the Benchmark average for sediment distributed as PS95.

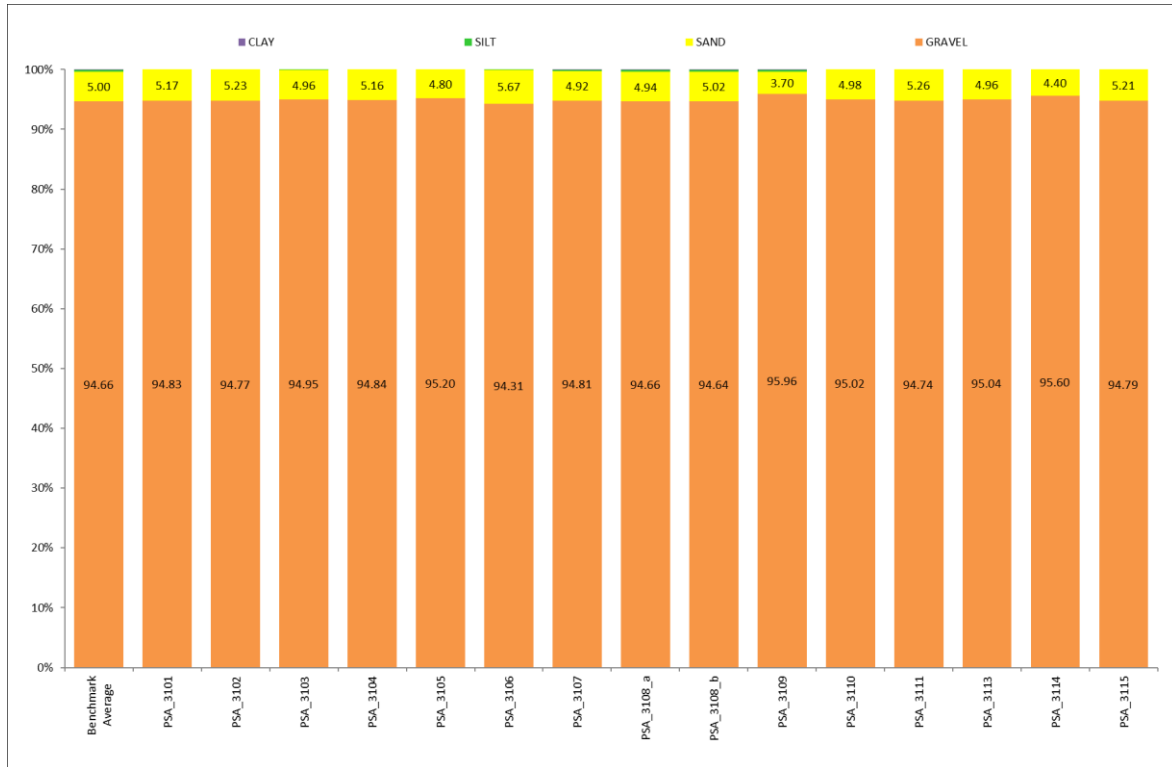


Figure 8 Bar charts showing the percentage gravel, sand, silt and clay recorded by each participating laboratory and the Benchmark average for PS95


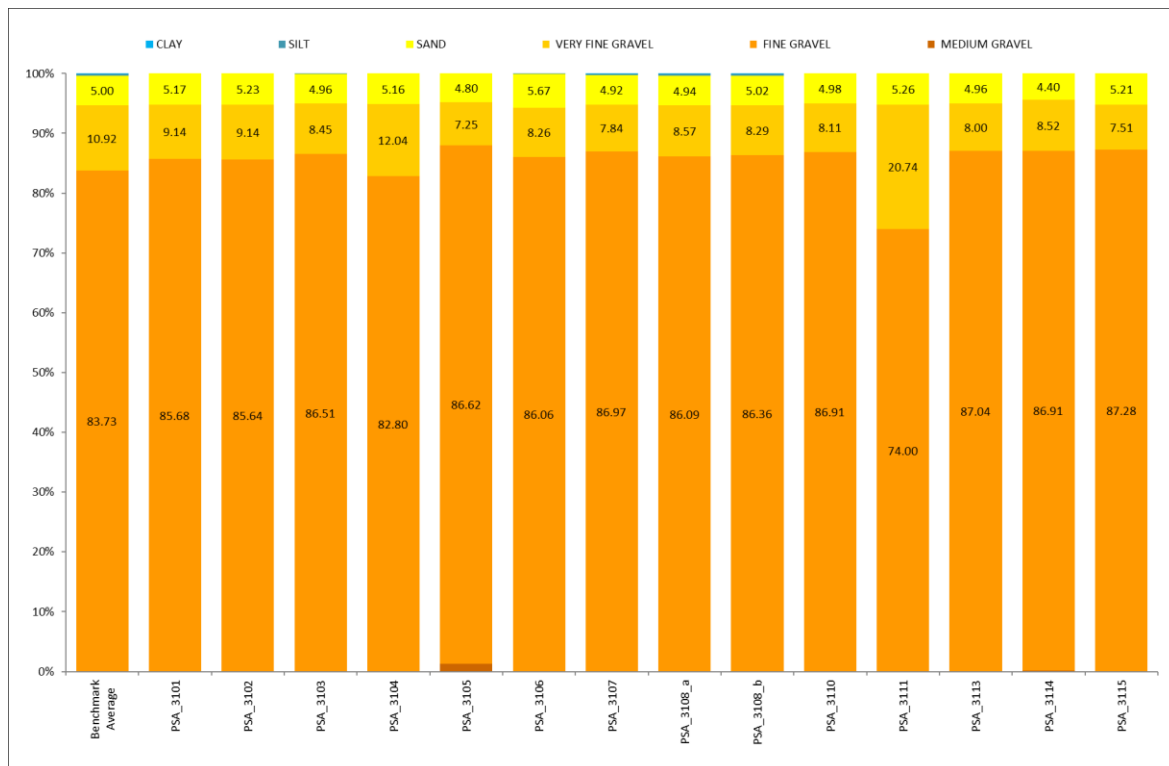


Figure 9 Bar charts showing the percentage medium, fine and very fine gravel, sand, silt and clay recorded by each participating laboratory and the Benchmark average for PS95.

3. APPENDICES

Appendix 1 – Participant Laser Replicate Graphs

Benchmark and Participant laser replicate data can be found in the associated embedded Excel file – PS95 Appendix 1.

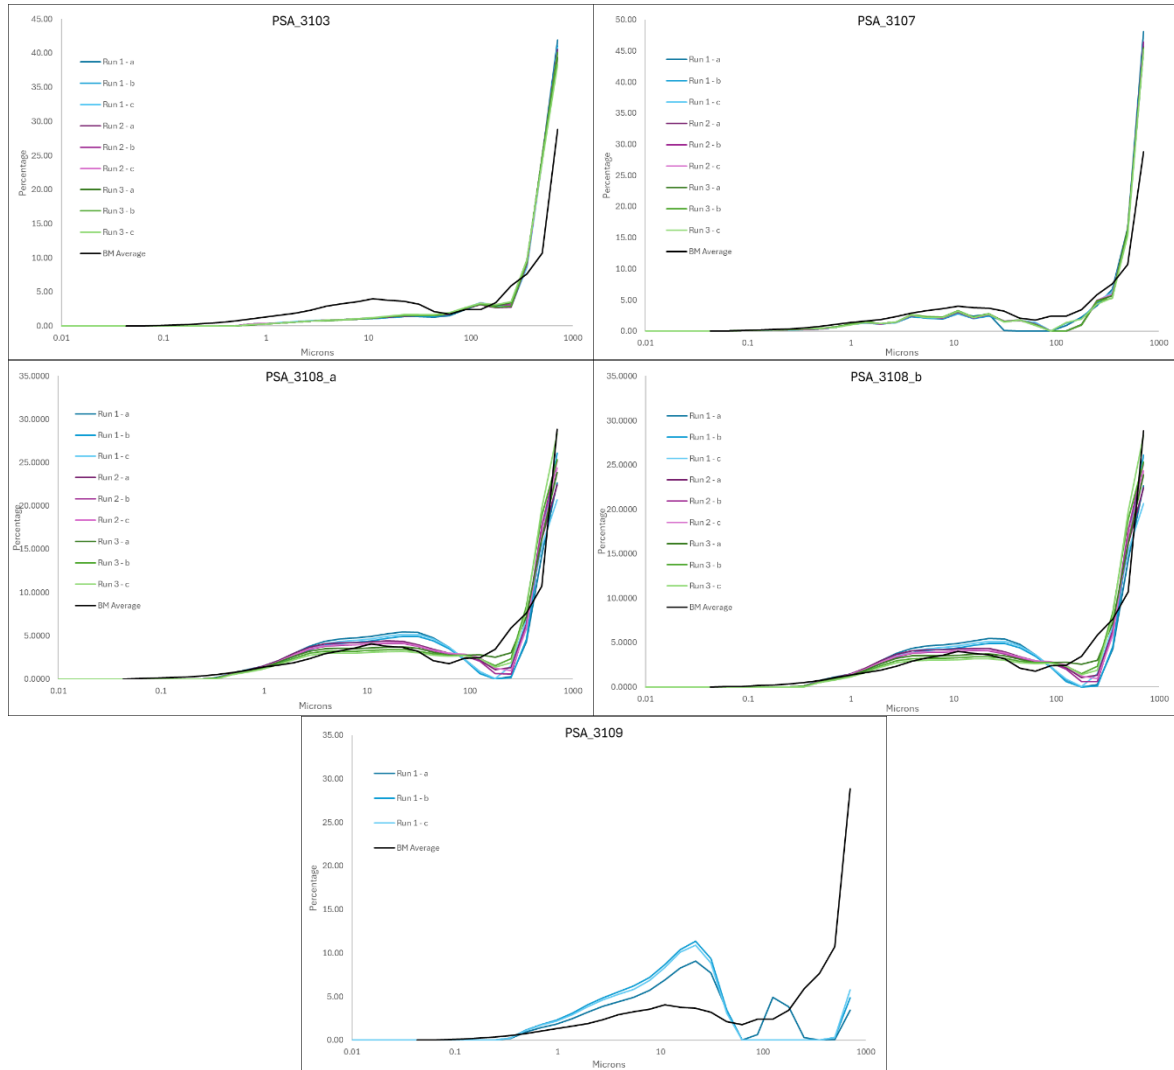

Appendix 2 – Gradistat output of size categories based on final merged data provided by each participant and the Benchmark Average for sediment distributed as PS95.

Benchmark and Participant data can be found in the associated embedded Excel file – PS95 Appendix 2.

Appendix 3 – Benchmark Lab and Participant Final Merged Data for sediment distributed as PS95.

Data can be found in the associated embedded Excel file – PS95 Appendix 3.

Appendix 4 – Individual comparison of participant and Benchmark sieve data for sediment distributed as PS95.

Data can be found in the associated embedded Excel file – PS95 Appendix 4.